

Product catalogue 2020

Clinical Diagnostics

Product catalogue 2020

Clinical Diagnostics

Content

R-Biopharm test systems at a glance	6
● Allergology	8
• Immunoblots	9
• ELISA – single allergen format	10
● Autoimmunity	12
• Autoimmune diseases	13
● Bacteriology	14
• <i>Bordetella</i> spp.	15
• <i>Borrelia</i> spp.	15
• <i>Campylobacter</i> spp.	16
• <i>Clostridium difficile</i>	17
• <i>Clostridium perfringens</i>	18
• <i>Escherichia coli</i>	18
• <i>Helicobacter pylori</i>	20
• <i>Legionella</i> spp.	21
• Methicillin-resistant/methicillin-sensitive <i>Staphylococcus aureus</i>	22
• <i>Mycoplasma</i> spp.	22
• <i>Salmonella</i> spp.	22
• <i>Treponema pallidum</i>	23
• <i>Yersinia enterocolitica</i>	23
• Various	24
• Accessories	25
● Gastroenterology	26
• Colon Cancer Prevention	27
• Inflammatory Bowel Disease	27
• Pancreatic Diagnostics	28
• Therapeutic Drug Monitoring (TDM)	29
● Mycology	30
• Fungi	31
• Accessories	31
● Parasitology	32
• <i>Cryptosporidium</i> spp.	33
• <i>Dientamoeba fragilis</i>	34
• <i>Entamoeba</i> spp.	35
• <i>Giardia lamblia</i>	36
• <i>Plasmodium</i> spp.	37
• Various	37
• Accessories	38

● Virology	40
• Adenovirus	41
• Astrovirus	42
• Cytomegalovirus	42
• Tick-borne Encephalitis	42
• Enterovirus	43
• Epstein-Barr-Virus	43
• Influenza	43
• Hantavirus	44
• Measles	44
• Mumps	44
• Norovirus	45
• Parainfluenza	46
• Parvovirus	46
• Rotavirus	47
• Respiratory Syncytial Virus & Human Metapneumovirus	48
• Sapovirus	48
• Accessories	49
● Systems	50
• Molecular diagnostics	51
• Immunoassay systems and evaluation software	51
• Rapid tests	51
• Blot systems and evaluation software	52
• Microspot array diagnostics	52
The R-Biopharm Group – contact us	54
General terms & conditions of R-Biopharm AG	55

R-Biopharm test systems at a glance



RIDASCREEN®

- ELISA for antigen and antibody detection
- Ready-to-use reagents
- Easy test procedure
- Standardized incubation time
- Possibility of processing on automated ELISA-systems
- Evaluation by the RIDASOFT® Win.NET software



RIDA®QUICK

- Reliable rapid test for antigen detection
- High sensitivity and specificity
- Agents distinguished by color
- 2 test formats:
 - Dipstick
 - Cassette



RIDA®GENE

- Real-time PCR
- Contains all necessary components
- Reliable results due to included extraction control
- Can be run on commonly used real-time PCR instruments



SeraSpot®

- Microspot array for antibody detection in autoimmune or infectious diseases
- For high throughput on common ELISA processors
- Ready-to-use reagents and universal test protocol
- Built-in controls and reference curve
- Cost and time efficient multiplex diagnostics



RIDA qLine®

- Quantitative immunoblot for antibody detection (IgE) in serum
- Various allergene panels available



Systems

- Flexible range of automated solutions
- Automated solutions for immunological and molecular tests
- ELISA automation solutions from small to high sample throughput
- Assistance in installation and routine by our application specialists



Allergology

Allergies are steadily increasing in industrialized countries. Nowadays, an allergy is defined as a specific hypersensitivity involving the immune system to substances which are actually harmless.

The four allergy types (type I – IV) originally classified by Coombs and Gell have meanwhile been joined by type V.

Type I allergy

The most frequent allergic reactions are type I reactions, which take place primarily on epithelial surfaces (skin, lungs, gastro-intestinal tract) and are characterized by the formation of specific immunoglobulin E against the allergens. These type I reaction is referred to as instant reaction and is the classic cause of allergic rhinitis, asthma and atopic dermatitis. The occurrence of this allergy type involves TH2 lymphocytes, which cause B lymphocytes to produce specific IgE antibodies, which are then bound to the surface of mast cells. On repeated contact with this allergen and cross-linking of mast cell-bound IgE antibodies, the mast cell secretes the biogenic amine histamine, which causes the symptoms of the allergy.

Type II and III allergies

Type II and III allergies are characterized by the formation of immunoglobulin M or G, with type II reactions acting against cell surfaces and type III reactions against soluble antigens. In type III reactions, the IgG antibodies form immunocomplexes with the allergens, which can cause

exogenic allergic alveolitis, for example. Furthermore, IgG antibodies against food stuff are suspect to mediate delayed food allergies.

Type IV and V allergies

Type IV reactions are cellular reactions which predominantly involve T lymphocytes. The granulomatous type V allergy can be regarded as a variant of type IV allergy, as it also triggers a cell-mediated immune reaction, but involves macrophages instead of T lymphocytes.

Allergy diagnostics

As a rule, the allergens are proteins from natural sources such as pollens, animal epithelia, insect venoms, foodstuffs, mites etc., although medicines such as penicillin and its derivatives can also trigger type I allergies. Patients show often a wide range of varying symptoms and sensitization patterns against several allergens. It is necessary to test a patient's blood whenever an allergic response or severe reaction is suspected. The allergy diagnostics of R-Biopharm AG offers two quantitative test methods for the antibody detection, the enzyme immunoassay (RIDASCREEN® Allergy ELISA) and the immunoblot (RIDA qLine® Allergy).



Immuno-
blot



ELISA



Accessories



Allergology

Immunoblots

Product	Description	Matrix	Tests	Art. No.
Immunoblots for antibody detection				
RIDA qLine®Allergy Panel 1	Immunoblot for quantitative determination of specific IgE in human serum or plasma (citrate) <ul style="list-style-type: none"> • standard curve on each strip • 13 inhalative and 7 food allergens • Test membranes (nitrocellulose) in reaction troughs 	Serum/Plasma (citrate)	10	A6142
RIDA qLine®Allergy Panel 2	Immunoblot for quantitative determination of specific IgE in human serum or plasma (citrate) <ul style="list-style-type: none"> • standard curve on each strip • 20 inhalative allergens • Test membranes (nitrocellulose) in reaction troughs 	Serum/Plasma (citrate)	10	A6242
RIDA qLine®Allergy Panel 3	Immunoblot for quantitative determination of specific IgE in human serum or plasma (citrate) <ul style="list-style-type: none"> • standard curve on each strip • 20 Food allergens • Test membranes (nitrocellulose) in reaction troughs 	Serum/Plasma (citrate)	10	A6342
RIDA qLine®Allergy Panel 4	Immunoblot for quantitative determination of specific IgE in human serum or plasma (citrate) <ul style="list-style-type: none"> • standard curve on each strip • 20 Allergens Pediatric panel • Test membranes (nitrocellulose) in reaction troughs 	Serum/Plasma (citrate)	10	A6442
Accessory				
RIDA®CCD-Inhibitor	Accessory for the inhibition of false positive results by cross-reactive anti-CCD IgE in human serum and plasma in in vitro diagnostics	Serum/Plasma (citrate)	25	ZA0601

Individual panels on request. Please ask your local distributor.



Allergology

ELISA – single allergen format

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassays for antibody detection				
RIDASCREEN® Total IgE	Enzyme immunoassay for the quantitative determination of total-IgE in serum <ul style="list-style-type: none"> Incl. standards and controls 	Serum	96	A0141
RIDASCREEN® Allergen Disc	1 allergen disc for an enzyme immunoassay <ul style="list-style-type: none"> For the quantitative determination of allergen-specific IgE/IgG in serum Without reagents Order units: <ul style="list-style-type: none"> Allergy Basic (3 x 8-well strips per allergen) Allergy Advance (12 x 8-well strip per panel of 8 allergens) 	Serum	1	A0049
RIDASCREEN® Spec. IgE Allergen Disc	1 allergen disc for an enzyme immunoassay <ul style="list-style-type: none"> For the quantitative determination of allergen-specific IgE in serum Incl. Reagents Order units: <ul style="list-style-type: none"> Allergy Active (individually preassembled plate; minimum number of allergens: 42) 	Serum	1	A0249
Accessories				
RIDASCREEN® Spec. IgE Reagents	Set of reagents for an enzyme immunoassay <ul style="list-style-type: none"> For the quantitative determination of allergen-specific IgE in serum Incl. standards and controls 	Serum	96	A0041
RIDASCREEN® Spec. IgE Reagents	Set of reagents for an enzyme immunoassay <ul style="list-style-type: none"> For the quantitative determination of allergen-specific IgE in serum Incl. standards and controls 	Serum	192	A0040





Autoimmunity

R-Biopharm offers you a new product line: *SeraSpot*®, the new microspot array for multiplex diagnostics of autoimmune diseases.

In autoimmunity, the immune system attacks structures of its own body. Depending on the attacked structure (e.g. nerves, joints, liver), the symptoms and thus the kind of disease vary. Today, around 81 different autoimmune diseases are known. These can be either localized, i.e. organ-specific, or systemic autoimmune diseases.

Many autoimmune diseases are characterized by autoantibodies. The autoantibodies are either directly pathogenic (e.g. anti-GBM) or disease associated. They can be valuable as prognostic markers (e.g. anti-AMA-M2), helpful in patient monitoring (e.g. anti-dsDNA) or necessary for differential diagnosis (e.g. anti-Mi2).

Importantly, the earlier the diagnosis of AID is made the better the outcome is for the patient. This is especially important in progressive e.g. rheumatic, fibrotic diseases that lead to irreversible deficits.

Diagnostics of autoimmune diseases

Autoantibody testing is a central element in the diagnosis and treatment of AID.

R-Biopharm offers *SeraSpot*®, a new microspot array for the diagnosis of autoimmune and infectious diseases.


Today, the *SeraSpot*® platform comprises 4 different microspot arrays plus the microspot array scanner for the diagnosis of connective tissue disease, autoimmune liver diseases or systemic vasculitis and goodpasture disease.



Microspot
array



Overview of SeraSpot® tests with respective target antigens:



Autoimmunity

Autoimmune diseases

Product	Description	Matrix	Tests	Art. No.
Microspot arrays				
SeraSpot® ANA-12 IgG	Specific detection of IgG antibodies against 12 nuclear and cytoplasmatic antigens	Serum/ plasma	1 x 48 1 x 96	SP-002-12 G-S6 SP-002-12 G-S12
SeraSpot® ANA-17 IgG	Specific detection of IgG antibodies against 17 nuclear and cytoplasmatic antigens	Serum/ plasma	1 x 48 1 x 96	SP-002-17 G-S6 SP-002-17 G-S12
SeraSpot® HepAk-7 IgG	Specific detection of IgG antibodies in autoimmune liver diseases	Serum/ plasma	1 x 48 1 x 96	SP-004-7 G-S6 SP-004-7 G-S12
SeraSpot® Vaskulitis-3 IgG	Specific detection of IgG antibodies in systemic vasculitis	Serum/ plasma	1 x 48 1 x 96	SP-003-3 G-S6 SP-003-3 G-S12





Bacteriology

Communicable diseases remain the most common death cause in emerging economies and are a huge public health concern in developed countries.

The health services are presented with a significant challenge in terms of diagnosis and treatment of infectious diseases. Effective use of the various diagnostic solutions can significantly improve the detection and control of infectious diseases caused by bacteria. The laboratory procedure must ensure that the information derived from the diagnostic test is reliable and delivered in a timely manner.

Diagnostic solutions in clinical bacteriology

Although the media culture is still the most established method in clinical bacteriology, there are a rising number of diagnostic bacteriology laboratories that deploy

commercial IVD kits in their procedures. The validated, reliable and rapid solutions offer a great advancement over the labour- and time-consuming culture method, in particular with respect to specificity and sensitivity.

The bacteriology test portfolio from R-Biopharm offers a wide range of solutions that meets the diagnostic and organizational needs of small to large laboratories. You may choose from a variety of systems to test for a wide range of parameters including *Legionella* spp., *Mycoplasma* spp., *Bordetella* spp. and *Clostridium difficile* spp..





Bacteriology

Bordetella spp.

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Bordetella	Multiplex Real-time PCR for the direct qualitative detection and differentiation of <i>Bordetella pertussis</i> , <i>Bordetella parapertussis</i> and <i>Bordetella holmesii</i> in human nasopharyngeal swabs and aspirates	Naso-pharyngeal swabs/ nasopharyngeal aspirates	100	PG2505
Enzyme immunoassays				
RIDASCREEN® Bordetella IgA Bordetella IgG Bordetella IgM	Specific detection of IgA, IgG or IgM antibodies against <i>Bordetella pertussis</i> and <i>Bordetella parapertussis</i> . Differentiation between infections and immune status after vaccination	Serum Serum Serum	96 96 96	K2511 K2521 K2531
RIDASCREEN® Bordetella PT IgA Bordetella PT IgG	Specific detection of IgA or IgG antibodies against toxin of <i>Bordetella pertussis</i> IgA- and IgG-analysis in international units (IU/ml)	Serum Serum	96 96	K2611 K2621



Borrelia spp.

Enzyme immunoassays				
RIDASCREEN® Borrelia IgG Borrelia IgM	Specific detection of IgG or IgM antibodies against <i>Borrelia burgdorferi sensu lato</i>	Serum Serum	96 96	K3221 K3231
Microspot arrays				
SeraSpot® Anti-Borrelia-10 IgG	Specific detection of IgG antibodies against <i>Borrelia burgdorferi sensu lato</i>	Serum/ plasma	1 x 96 10 x 96	SP-006-10 G-S12 SP-006-10 G-S120
SeraSpot® Anti-Borrelia-10 IgM	Specific detection of IgM antibodies against <i>Borrelia burgdorferi sensu lato</i>	Serum/ plasma	1 x 96 10 x 96	SP-006-10 M-S12 SP-006-10 M-S120





Bacteriology

Campylobacter spp.

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Bacterial Stool Panel	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Salmonella</i> spp., <i>Campylobacter</i> spp. and <i>Yersinia enterocolitica</i> in human stool samples	Stool	100	PG2405
RIDA®GENE Bacterial Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Salmonella</i> spp., <i>Campylobacter</i> spp., EIEC/ <i>Shigella</i> spp. and STEC in human stool samples	Stool	100	PG2415
Enzyme immunoassay				
RIDASCREEN® <i>Campylobacter</i>	Enzyme immunoassay for the detection of <i>Campylobacter jejuni</i> and <i>Campylobacter coli</i> in human stool samples	Stool	96	C2401
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® <i>Campylobacter</i> Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP2404
Rapid test				
RIDA®QUICK <i>Campylobacter</i>	Immunochromatographic lateral flow rapid assay for the detection of <i>Campylobacter jejuni</i> und <i>Campylobacter coli</i> in human stool samples Single pouched cassettes	Stool	25	N2403
Controls for RIDA®QUICK				
RIDA®QUICK <i>Campylobacter</i> Control	Positive control	–	1.8 ml	NP2404



***Clostridium difficile***

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE CD Toxin A/B	Multiplex real-time PCR for the direct qualitative detection of <i>Clostridium difficile</i> toxin genes A (tcdA) and B (tcdB) in human stool and culture samples	Stool/ cultures	100	PG0825
RIDA®GENE Clostridium difficile	Multiplex real-time PCR for the direct qualitative detection of <i>Clostridium difficile</i> and <i>Clostridium difficile</i> toxin genes A (tcdA) and B (tcdB) in human stool and culture samples	Stool/ cultures	100	PG0835
RIDA®GENE Hospital Stool Panel	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus (genogroup I and II), Rotavirus and <i>Clostridium difficile</i> toxin genes A (tcdA) and B (tcdB) in human stool samples	Stool	100	PG0705
Enzyme immunoassay				
RIDASCREEN® Clostridium difficile GDH	Enzyme immunoassay for the detection of glutamate dehydrogenase of <i>Clostridium difficile</i> in human stool samples	Stool	96	C0701
RIDASCREEN® Clostridium difficile Toxin A/B	Enzyme immunoassay for the detection of toxin A and B of <i>Clostridium difficile</i>	Stool	96	C0801
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Clostridium difficile GDH Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP0704
RIDASCREEN® Clostridium difficile Toxin A/B Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP0804
Rapid test				
RIDA®QUICK Clostridium difficile GDH	Immunochromatographic lateral flow rapid assay for the detection of <i>Clostridium difficile</i> GDH Single pouched cassettes	Stool	25	N0703
RIDA®QUICK Clostridium difficile Toxin A/B	Immunochromatographic lateral flow rapid assay for the detection of Toxins A and B of <i>C. difficile</i> Single pouched cassettes	Stool	25	N0803
Controls for RIDA®QUICK				
RIDASCREEN® Clostridium difficile GDH Control	Positive control	–	1.8 ml	NP0704
RIDA®QUICK Clostridium difficile Toxin A/B Control	Positive control	–	1.8 ml	NP0804





Bacteriology

Clostridium perfringens

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassay				
RIDASCREEN® <i>Clostridium perfringens</i> Enterotoxin	Enzyme immunoassay for detection of enterotoxin of <i>Clostridium perfringens</i> in human stool samples	Stool	96	C0601
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® <i>Clostridium perfringens</i> Enterotoxin Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP0604



Escherichia coli

Real-time PCR				
RIDA®GENE EHEC/EPEC	Multiplex real-time PCR for the direct qualitative detection and differentiation of EHEC, STEC, EPEC and EIEC/ <i>Shigella</i> spp. in human stool and culture samples	Stool/ cultures	100	PG2205
RIDA®GENE EAEC	Multiplex real-time PCR for the direct qualitative detection and differentiation of enteroaggregative <i>E. coli</i> (EAEC) in human stool samples and cultures	Stool/ cultures	100	PG2215
RIDA®GENE ETEC/EIEC	Multiplex real-time PCR for the direct qualitative detection and differentiation of ETEC and EIEC/ <i>Shigella</i> spp. in human stool samples and cultures	Stool/ cultures	100	PG2225
RIDA®GENE <i>E. coli</i> Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of shigatoxin genes (stx1 and stx2) of shigatoxin producing <i>E. coli</i> (STEC) and EPEC in human stool samples	Stool	100	PG2285
RIDA®GENE Bacterial Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Salmonella</i> spp., <i>Campylobacter</i> spp., <i>EIEC/Shigella</i> spp. and STEC in human stool samples	Stool	100	PG2415





Bacteriology

Escherichia coli

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassay				
RIDASCREEN® Verotoxin	Enzyme immunoassay for the detection of verotoxins 1 and 2 (shigatoxins 1 and 2) of <i>Escherichia coli</i> in a stool enrichment	mTSB-Bouillon	96	C2201
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Verotoxin Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP2204
Rapid test				
RIDA®QUICK Verotoxin/O157 Combi	Immunochromatographic rapid assay for the detection of verotoxins and/or <i>E. coli</i> O157 in a stool enrichment Single pouched cassettes	mTSB-Buillon	20	N2203
Controls for RIDA®QUICK				
RIDA®QUICK Verotoxin/O157 Combi Control	Positive control	–	1.8 ml	NP2204
Enrichment broth				
Accessory				
RIDA® Enrichment broth	mTSB-buillon with Mitomycin C for the enrichment of verotoxin (shigatoxin)-producing <i>E. coli</i> bacteria	–	100	Z1000
RIDA® Enrichment broth	mTSB-buillon with Mitomycin C for the enrichment of verotoxin (shigatoxin)-producing <i>E. coli</i> bacteria	–	25	Z1003





Bacteriology

Helicobacter pylori

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE <i>Helicobacter pylori</i>	Multiplex real-time PCR for the direct qualitative detection of <i>Helicobacter pylori</i> and its resistance to clarithromycin in human biopsy tissue	Biopsy	100	PG2305
Microspot arrays				
SeraSpot® Anti- <i>Helicobacter</i> -6 IgA	Specific detection of IgA antibodies against <i>Helicobacter pylori</i>	Serum/ plasma	1 x 48 1 x 96	SP-007-6 A-S6 SP-007-6 A-S12
SeraSpot® Anti- <i>Helicobacter</i> -6 IgG	Specific detection of IgG antibodies against <i>Helicobacter pylori</i>	Serum/ plasma	1 x 48 1 x 96	SP-007-6 G-S6 SP-007-6 G-S12
Enzyme immunoassays				
RIDASCREEN® <i>Helicobacter</i> IgA <i>Helicobacter</i> IgG	Specific detection of IgA or IgG antibodies against <i>Helicobacter pylori</i>	Serum Serum	96 96	K2311 K2321
RIDASCREEN® <i>Helicobacter</i>	Enzyme immunoassay for the detection of <i>Helicobacter pylori</i> in human stool samples	Stool	96	C2302
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® H. <i>pylori</i> Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP2304
Rapid test				
RIDA®QUICK <i>Helicobacter</i>	Immunochromatographic lateral flow rapid assay for the detection of <i>Helicobacter pylori</i> in human stool samples Single pouched cassettes	Stool	25	N2303
Controls for RIDA®QUICK				
RIDA®QUICK <i>Helicobacter</i> Control	Positive control	–	1.8 ml	NP2304





Bacteriology

Legionella spp.

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Legionella	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Legionella</i> spp. and <i>Legionella pneumophila</i> in human sputum, BAL and tracheal secretion	Sputum/ BAL/tracheal secretion	100	PG8005
Enzyme immunoassay				
RIDASCREEN® Legionella	Enzyme immunoassay for the detection of <i>Legionella pneumophila</i> in human urine samples	Urine	96	C8001
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Legionella Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP8004
Immunofluorescence assay				
RIDA® FLUOR Legionella IgG (3 Pools)	Row 1: SG 1 - 6 Row 2: SG 7 - 14 Row 3: L. boz-dum-gor-jord-longb-mic Immunofluorescence assay for detection of IgG antibodies against <i>Legionella pneumophila</i> serogroup 1 - 14 and six non-pneumophila species of <i>Legionella</i>	Serum	10 x 30	I8521
Controls for immunofluorescence assays				
RIDA® FLUOR Legionella IgG Negative control	Negative control IgG	Serum	0.2 ml	I8521 C00
RIDA® FLUOR Legionella IgG Positive control	Positive control IgG	Serum	0.2 ml	I8521 C01





Bacteriology

Methicillin-resistant/methicillin-sensitive *Staphylococcus aureus*

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE MRSA	Multiplex real-time PCR for the direct qualitative detection of MRSA in swab specimens (nose, nose/throat, wound, axilla, groin, perianal) and culture samples	Swab specimens (nose, nose/throat, wound, axilla, groin, perianal)/cultures	100	PG0605
RIDA®GENE PVL	Multiplex real-time PCR for the direct qualitative detection of the PVL-gene (Panton-Valentine leukocidine) in human swab specimens (nose, wound) and culture samples	Swab specimens (nose, wound)/cultures	100	PG0645



Mycoplasma spp.

Real-time PCR				
RIDA®GENE STI Mycoplasma Panel	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Mycoplasma hominis</i> , <i>Mycoplasma genitalium</i> and <i>Ureaplasma urealyticum/parvum</i> in human genital swabs and urine	Genital swab/urine	100	PG4945
RIDA®GENE Mycoplasma pneumoniae	Multiplex real-time PCR for the direct qualitative detection of <i>Mycoplasma pneumoniae</i> in human sputum, BAL and tracheal secretion	Sputum/BAL/tracheal secretion	100	PG4305
Enzyme immunoassays				
RIDASCREEN® Mycoplasma pneumoniae IgA	Specific detection of IgA, IgG or IgM antibodies against <i>Mycoplasma pneumoniae</i>	Serum	96	K4311
Mycoplasma pneumoniae IgG		Serum	96	K4321
Mycoplasma pneumoniae IgM		Serum	96	K4331



Salmonella spp.

Real-time PCR				
RIDA®GENE Bacterial Stool Panel	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Salmonella</i> spp., <i>Campylobacter</i> spp. and <i>Yersinia enterocolitica</i> in human stool samples	Stool	100	PG2405
RIDA®GENE Bacterial Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Salmonella</i> spp., <i>Campylobacter</i> spp., EIEC/ <i>Shigella</i> spp. and STEC in human stool samples	Stool	100	PG2415





Bacteriology

Treponema pallidum

Product	Description	Matrix	Tests	Art. No.
Microspot arrays				
SeraSpot® Anti-Treponema-4 IgG	Specific detection of IgG antibodies against <i>Treponema pallidum</i>	Serum/ plasma	1 x 48 1 x 96	SP-010-4 G-S6 SP-010-4 G-S12
SeraSpot® Anti-Treponema-4 IgM	Specific detection of IgM antibodies against <i>Treponema pallidum</i>	Serum/ plasma	1 x 48 1 x 96	SP-010-4 M-S6 SP-010-4 M-S12



Yersinia enterocolitica

Real-time PCR				
RIDA®GENE Bacterial Stool Panel	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Salmonella</i> spp., <i>Campylobacter</i> spp. and <i>Yersinia enterocolitica</i> in human stool samples	Stool	100	PG2405
Microspot arrays				
SeraSpot® Anti-Yersinia-6 IgA	Specific detection of IgA antibodies against <i>Yersinia enterocolitica</i>	Serum/ plasma	1 x 48 1 x 96	SP-005-6 A-S6 SP-005-6 A-S12
SeraSpot® Anti-Yersinia-6 IgG	Specific detection of IgG antibodies against <i>Yersinia enterocolitica</i>	Serum/ plasma	1 x 48 1 x 96	SP-005-6 G-S6 SP-005-6 G-S12





Bacteriology

Various

Product	Description	Matrix	Tests	Art. No.
Akkermansia muciniphila				
Real-time PCR				
RIDA®GENE Akkermansia muciniphila	Multiplex real-time PCR for the direct qualitative or quantitative detection of <i>Akkermansia muciniphila</i> in human stool samples	Stool	100	PG0145
Diphtherie				
Enzyme immunoassay				
RIDASCREEN® Diphtherie IgG	Specific detection of IgG antibodies against diphtheria toxoid. Analysis in international units (IU/ml)	Serum	96	K3821
Faecalibacterium prausnitzii				
Real-time PCR				
RIDA®GENE Faecalibacterium prausnitzii	Multiplex real-time PCR for the direct qualitative or quantitative detection of <i>Faecalibacterium prausnitzii</i> in human stool samples	Stool	100	PG0155
Bacteroides/Clostridium Cluster XIVa – Real-time PCR				
RIDA®GENE Gut Balance	Multiplex real-time PCR for the direct qualitative or quantitative detection and differentiation of <i>Bacteroides</i> and <i>Clostridium</i> Cluster XIVa in human stool samples	Stool	100	PG0105
Tetanus				
Enzyme immunoassay				
RIDASCREEN® Tetanus IgG	Specific detection of IgG antibodies against tetanus toxoid. Analysis in international units (IU/ml)	Serum	96	K3721



Accessories

Product	Description	Matrix	Tests	Art. No.
Color compensation				
RIDA®GENE Color Compensation Kit I	To generate a Color Compensation File for 3- and 4-plex RIDA®GENE real-time PCR experiments on the LightCycler®480II*	–	3	PG0001
RIDA®GENE Color Compensation Kit II	To generate a Color Compensation File for RIDA®GENE real-time PCR experiments on the LightCycler® 1.5/2.0	–	3	PG0002
RIDA®GENE Color Compensation Kit IV	To generate a Color Compensation File for 5-plex RIDA®GENE real-time PCR experiments on the LightCycler® 480II**	–	3	PG0004
DNA/RNA extraction				
RIDA® Xtract	Spin-filter based extraction kit for the simultaneous isolation and purification of DNA and RNA in various matrices (serum/ plasma/ cerebral fluid/ cell culture supernatant/ other cell free body fluids (e.g. urine)/ swabs/tissue biopsies/stool)	see description	250 pre- parations	PGZ001
Accessory for RIDASCREEN® antibody detection tests				
RIDA® RF-Absorbens	Anti-human IgG for absorption of rheumatoid factors (RF) and IgG antibodies in human serum or plasma	Serum/ plasma	100	Z0202



* For RIDAGENE products of the generation 1.0.

** For RIDAGENE products of the generation 2.0.



Gastroenterology

Our gastroenterology product portfolio is not only dedicated to the advanced diagnosis of gut-related diseases such as inflammatory bowel disease or pancreatic insufficiency but also perfectly suited for the prevention of gut-related diseases such as colon cancer.

The ELISA tests are suited for single plate or medium-high-throughput analysis on automated readers. Below, you can find the biological markers and their diagnostic relevance at a glance.

Biomarkers for clinical diagnostics

Biological markers (biomarkers) are measurable indicators for specific conditions. The following biomarkers are relevant in gastroenterology:

- **Calprotectin** is a highly specific indicator of gastrointestinal inflammation which is used for the differentiation of IBD and IBS and for treatment monitoring.
- **Haemoglobin** is a very efficient marker for colon cancer screening. The antibody-based tests RIDASCREEN® Haemoglobin and RIDASCREEN®

Haemo-/Haptoglobin Complex are more specific than Guaiac-based tests. A combined testing of both parameters increases the probability to detect adenomas.

- **α 1-antitrypsin and sIgA** indicate the integrity of the gut wall. This is relevant for monitoring and diagnosing a leaky gut syndrome.
- **Pancreatic elastase and pankrin** are used for the detection of pancreatic insufficiency and pancreatitis.

Therapeutic drug monitoring

Therapeutic drug monitoring of infliximab (IFX), adalimumab (ADM), vedolizumab (VDZ) and golimumab (GLM) supports the treatment optimization and the reduction of treatment costs.



ELISA



Lateral Flow



Accessories



Colon Cancer Prevention

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassays				
RIDASCREEN® Haemoglobin	Enzyme immunoassay for the quantitative determination of haemoglobin	Stool	96	G09030
RIDASCREEN® Haemo-/Haptoglobin Complex	Enzyme immunoassay for the quantitative determination of haemoglobin/haptoglobin complex	Stool	96	G09031
Stool collection tubes				
RIDA® TUBE Haemoglobin	For collection and preparation of stool samples, • only use with RIDASCREEN® Haemoglobin (G09030) and RIDASCREEN® Haemo-/Haptoglobin Complex (G09031)	–	50	GZ3012



Inflammatory Bowel Disease

Enzyme immunoassays				
RIDASCREEN® α_1 -Antitrypsin	Enzyme immunoassay for the quantitative determination of α_1 -Antitrypsin	Stool	96	G09034
RIDASCREEN® sIgA	Enzyme immunoassay for the quantitative determination of secretoric IgA	Stool	96	G09035
Stool collection tubes				
RIDA® TUBE	For collection and preparation of stool samples, • unfilled; to use after internal validation	–	50	GZ3013
Enzyme immunoassay				
RIDASCREEN® Calprotectin	Enzyme immunoassay for the quantitative determination of calprotectin	Stool	96	G09036
Stool collection tubes				
RIDA® TUBE Calprotectin	For the collection and preparation of stool samples, • only for use with RIDASCREEN® Calprotectin (G09036)	–	50	GZ3016





Gastroenterology

Pancreatic Diagnostics

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassays				
Pancreatic Elastase ELISA	Enzyme immunoassay for the quantitative determination of pancreatic elastase	Stool	96	G09038
Pancreatic Elastase ELISA (SK15)	Enzyme immunoassay for the quantitative determination of pancreatic elastase; additional standard (SK15)	Stool	96	G09040
Stool collection tubes				
Stool Preparation Set	For collection and preparation of stool samples, • only use with Pancreatic Elastase ELISA G09038 and G09040	Serum/ Plasma	45	GZ3008





Therapeutic Drug Monitoring (TDM)

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassays				
RIDASCREEN® ADM Monitoring	Enzyme immunoassay for the quantitative determination of adalimumab (ADM)	Serum/ Plasma	96	G09043
RIDASCREEN® Anti-ADM Antibodies	Enzyme immunoassay for the quantitative determination of antibodies to adalimumab (ADM)	Serum/ Plasma	96	G09044
RIDASCREEN® IFX Monitoring	Enzyme immunoassay for the quantitative determination of infliximab (IFX) and its biosimilars	Serum/ Plasma	96	G09041
RIDASCREEN® Anti-IFX Antibodies	Enzyme immunoassay for the quantitative determination of antibodies to infliximab (IFX) and its biosimilars	Serum/ Plasma	96	G09042
RIDASCREEN® VDZ Monitoring	Enzyme immunoassay for the quantitative determination of vedolizumab (VDZ)	Serum/ Plasma	96	G09045
RIDASCREEN® GLM Monitoring	Enzyme immunoassay for the quantitative determination of golimumab (GLM)	Serum/ Plasma	96	G09047
Rapid tests				
RIDA®QUICK ADM Monitoring	Immunochromatographic lateral flow assay for the quantitative determination of adalimumab (ADM)	Serum/ Plasma	25	GN3043
RIDA®QUICK IFX Monitoring	Immunochromatographic lateral flow assay for the quantitative determination of infliximab (IFX) and its biosimilars	Serum/ Plasma	25	GN3041
Positive controls for RIDA®QUICK				
RIDA®QUICK ADM Monitoring Control Set	Positive controls • accessory for GN3043	–	–	GP3043
RIDA®QUICK IFX Monitoring Control Set	Positive controls • accessory for GN3041	–	–	GP3041





Mycology

The incidence of fungal infections is increasing, based on some recent evidence. It has been calculated that infections with fungi occur in approximately a billion people each year.

Although fungi play many essential roles in human homeostasis, they may also constitute health burden for certain groups of patients. When the host–fungal pathogen balance is disturbed, a fungal infection may lead to serious consequences. Proper detection of the growth of the fungal agents is therefore of high importance in clinical microbiology.

Pneumocystis jirovecii does not cause any harm in healthy people and is widely spread among the normal population. However, immunocompromised people

infected with *Pneumocystis jirovecii*, develop pneumonia with symptoms including dry cough, shortness of breath, tachypnoe and fever. *Pneumocystis jirovecii* causes respiratory infections and is the most common opportunistic illness in HIV-infected people.

Diagnostic solutions for mycology

The mycology tests portfolio from R-Biopharm offers PCR technology that meet the diagnostic needs of laboratories.



Real-time
PCR



Accessories





Mycology

Fungi

Product	Description	Matrix	Tests	Art. No.
<i>Pneumocystis jirovecii</i>	Real-time PCR			
RIDA® GENE Pneumocystis jirovecii	Multiplex real-time PCR for the direct qualitative or quantitative detection of <i>Pneumocystis jirovecii</i> from BAL	BAL	100	PG1905



Accessories

DNA/RNA extraction				
RIDA® Xtract	Spin-filter based extraction kit for the simultaneous isolation and purification of DNA and RNA in various matrices (serum/ plasma/ cerebral fluid/ cell culture supernatant/ other cell free body fluids (e.g. urine)/ swabs/tissue biopsies/stool)	see description	250 preparations	PGZ001





Parasitology

Infections with parasites are very common in tropical climate regions where the most common example of such an infection is malaria. In non-tropical areas, the most typical diseases caused by parasites are trichomoniasis, giardiasis, cryptosporidiosis, amebiasis and toxoplasmosis.

Parasitic infections are caused by three types of organisms: protozoa, helminths and ectoparasites. Infections with protozoa can occur by, for instance, drinking water containing the protozoa organisms' cells or through food that was undercooked. *Giardia lamblia*, *Cryptosporidium parvum*, *Entamoeba histolytica* and *Dientamoeba fragilis* are the most important diarrhea-causing protozoa.

Due to the ease of spread, fast and reliable diagnosis of a parasitic infection at an early stage is crucial for an effective therapy. Immunoassays and molecular

diagnostics enable detection and differentiation of parasitic infections sooner than traditional methods, such as microscopy.

Innovative diagnostic solutions for parasitology

R-Biopharm offers various technologies for parasitology that meet the diagnostic and organizational needs of small to large laboratories. You may choose from different diagnostic systems to test for a variety of parasites including *Entamoeba*, *Giardia* and *Cryptosporidium*. We also offer a parasitic stool panel.



Real-time
PCR



ELISA



Lateral
Flow



Accessories





Parasitology

Cryptosporidium spp.

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Parasitic Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> , <i>Cryptosporidium</i> spp. and <i>Dientamoeba fragilis</i> in human stool samples	Stool	100	PG1715
RIDA®GENE Parasitic Stool Panel II	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> and <i>Cryptosporidium</i> spp. in human stool samples	Stool	100	PG1725
Enzyme immunoassay				
RIDASCREEN® Cryptosporidium	Enzyme immunoassay for the detection of <i>Cryptosporidium parvum</i> and <i>Cryptosporidium hominis</i> in human stool samples	Stool	96	C1201
Reference control for RIDASCREEN® ELISA				
RIDASCREEN® Cryptosporidium Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP1204





Parasitology

Cryptosporidium spp.

Product	Description	Matrix	Tests	Art. No.
Rapid tests				
RIDA®QUICK <i>Cryptosporidium</i>	Immunochromatographic rapid assay for the detection of <i>Cryptosporidium parvum</i> and <i>Cryptosporidium hominis</i> in human stool samples Single pouched cassettes	Stool	20	N1203
RIDA®QUICK <i>Cryptosporidium</i> /Giardia Combi	Immunochromatographic rapid assay for the detection of <i>Cryptosporidium parvum</i> , <i>Cryptosporidium hominis</i> and/or <i>Giardia lamblia</i> in human stool samples Single pouched cassettes	Stool	20	N1123
RIDA®QUICK <i>Cryptosporidium</i> /Giardia/Entamoeba Combi	Immunochromatographic rapid assay for the detection of <i>Cryptosporidium parvum</i> , <i>Cryptosporidium hominis</i> and/or <i>Giardia lamblia</i> in human stool samples Single pouched cassettes	Stool	20	N1723
Controls for RIDA®QUICK				
RIDA®QUICK Parasite Combi Control	Positive control	–	1.8 ml	NP1704



Dientamoeba fragilis

Real-time PCR				
RIDA®GENE Parasitic Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> , <i>Cryptosporidium</i> spp. and <i>Dientamoeba fragilis</i> in human stool samples	Stool	100	PG1715





Parasitology

Entamoeba spp.

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Parasitic Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> , <i>Cryptosporidium</i> spp. and <i>Dientamoeba fragilis</i> in human stool samples	Stool	100	PG1715
RIDA®GENE Parasitic Stool Panel II	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> and <i>Cryptosporidium</i> spp. in human stool samples	Stool	100	PG1725
Entamoeba Enzyme immunoassays				
RIDASCREEN® Entamoeba histolytica IgG	Specific detection of IgG antibodies against <i>Entamoeba histolytica</i>	Serum	96	K1721
RIDASCREEN® Entamoeba	Enzyme immunoassay for the detection of <i>Entamoeba histolytica</i> / <i>Entamoeba dispar</i> in human stool samples	Stool	96	C1701
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Entamoeba Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP1704
Rapid test				
RIDA®QUICK Entamoeba	Immunochromatographic rapid assay for the detection of <i>Entamoeba histolytica</i> / <i>Entamoeba dispar</i> in human stool samples Single pouched cassettes	Stool	20	N1703
RIDA®QUICK Cryptosporidium/Giardia/ Entamoeba Combi	Immunochromatographic rapid assay for the detection of <i>Cryptosporidium</i> and/or <i>Giardia</i> and/or <i>Entamoeba</i> in human stool samples Single pouched cassettes	Stool	20	N1723
Controls for RIDA®QUICK				
RIDA®QUICK Parasite Combi Control	Positive control	–	1.8 ml	NP1704





Parasitology

Giardia lamblia

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Parasitic Stool Panel I	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> , <i>Cryptosporidium</i> spp. and <i>Dientamoeba fragilis</i> in human stool samples	Stool	100	PG1715
RIDA®GENE Parasitic Stool Panel II	Multiplex real-time PCR for the direct qualitative detection and differentiation of <i>Giardia lamblia</i> , <i>Entamoeba histolytica</i> and <i>Cryptosporidium</i> spp. in human stool samples	Stool	100	PG1725
Enzyme immunoassay				
RIDASCREEN® Giardia	Enzyme immunoassay for the detection of <i>Giardia lamblia</i> in human stool samples	Stool	96	C1101
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Giardia Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP1104
Rapid test				
RIDA®QUICK Giardia	Immunochromatographic rapid assay for the detection of <i>Giardia lamblia</i> Single pouched cassettes	Stool	20	N1103
RIDA®QUICK Cryptosporidium/Giardia Combi	Immunochromatographic rapid assay for the detection of <i>Cryptosporidium parvum</i> , <i>Cryptosporidium hominis</i> and/or <i>Giardia lamblia</i> in human stool samples Single pouched cassettes	Stool	20	N1123
RIDA®QUICK Cryptosporidium/Giardia/ Entamoeba Combi	Immunochromatographic rapid assay for the detection of <i>Cryptosporidium parvum</i> , <i>Cryptosporidium hominis</i> and/or <i>Giardia lamblia</i> in human stool samples Single pouched cassettes	Stool	20	N1723
Controls for RIDA®QUICK				
RIDA®QUICK Parasite Combi Control	Positive control	–	1.8 ml	NP1704





Parasitology

Plasmodium spp.

Product	Description	Matrix	Tests	Art. No.
Rapid test				
RIDA®QUICK Malaria	Immunochromatographic rapid assay for the detection of Plasmodia species in human whole blood samples Single pouched cassettes	Blood	25	N7006
RIDA®QUICK Malaria	Immunochromatographic rapid assay for the detection of Plasmodia species in human whole blood samples Single pouched cassettes	Blood	5	N7007
Controls for RIDA®QUICK				
RIDA®QUICK Malaria Positive Control	Positive control	–	1.8 ml	NP7004



Various

<i>Trichomonas vaginalis</i>	Real-time PCR			
RIDA®GENE Trichomonas vaginalis	Multiplex real-time PCR for the direct qualitative detection of <i>Trichomonas vaginalis</i> in human genital swabs and urine	Genital swab/Urine	100	PG4975
<i>E. granulosus/multiloculra</i> s	Enzyme immunoassay			
RIDASCREEN® Echinococcus IgG	Specific detection of IgG antibodies against <i>Echinococcus granulosus</i> and <i>Echinococcus multilocularis</i>	Serum	96	K7621
<i>Leshmania infantum</i>	Enzyme immunoassay			
RIDASCREEN® Leshmania IgG	Specific detection of IgG antibodies against <i>Leishmania infantum</i>	Serum	96	K7321
<i>Taenia solium</i>	Enzyme immunoassay			
RIDASCREEN® Taenia solium IgG	Specific detection of IgG antibodies against the larval forms of <i>Taenia solium</i> (cysticercosis)	Serum	96	K7721
<i>Toxocara canis</i>	Enzyme immunoassay			
RIDASCREEN® Toxocara IgG	Specific detection of IgG antibodies against <i>Toxocara canis</i>	Serum	96	K7421
<i>Trichinella spiralis</i>	Enzyme immunoassay			
NovaLisa™Trichinella spiralis	Specific detection of IgG antibodies against <i>Trichinella spiralis</i>	Serum/Plasma (citrate)	96	TRIG0480





Parasitology

Accessories

Product	Description	Matrix	Tests	Art. No.
Accessories				
Color compensation				
RIDA®GENE Color Compensation Kit I	To generate a Color Compensation File for 3- and 4-plex RIDA®GENE real-time PCR experiments on the LightCycler®480II*	–	3	PG0001
RIDA®GENE Color Compensation Kit II	To generate a Color Compensation File for RIDA®GENE real-time PCR experiments on the LightCycler® 2.0	–	3	PG0002
RIDA®GENE Color Compensation Kit IV	To generate a Color Compensation File for RIDA®GENE real-time PCR experiments on the LightCycler® 480II**	–	3	PG0004
DNA/RNA extraction				
RIDA® Xtract	Spin-filter based extraction kit for the simultaneous isolation and purification of DNA and RNA in various matrices (serum/ plasma/ cerebral fluid/ cell culture supernatant/ other cell free body fluids (e.g. urine)/ swabs/tissue biopsies/stool)	see description	250 preparations	PGZ001



* For RIDAGENE products of the generation 1.0.

** For RIDAGENE products of the generation 2.0.



Virology

Clinical virology has been rapidly changing during the last years.

A modern clinical virology laboratory performs various tests, such as rapid antigen testing, serology or molecular diagnostics in order to provide the best services to the healthcare institutions and patients.

Effective use of these diagnostic platforms enables the timely detection and control of infectious diseases caused by viral agents. We offer a rich portfolio of parameters and technologies for clinical virology, with a particular focus on viruses causing gastrointestinal infections and respiratory infections.


Norovirus diagnostics: fast diagnostics in outbreaks – always on the forefront

Noroviruses are a major cause of gastroenteritis world-wide with an estimated 23 million cases a year in the USA. They are frequently the reason of outbreaks in communal facilities, for instance nursing homes, hospitals, prisons and cruise ships. Since norovirus outbreaks are reported more often than outbreaks caused by bacterial pathogens, they may have a considerable impact on public health.

The reliable norovirus diagnostic tests from R-Biopharm help clinical laboratories of all sizes detect the infection with norovirus in a simple and fast manner. Depending on their needs, laboratories may pick from our ELISA, rapid tests or PCR product portfolio.

Innovative diagnostic solutions for virology

Our virology catalogue offers technologies that meet the diagnostic and organizational needs of small to large laboratories. You may choose from different systems to test for a variety of viral pathogens including Norovirus, Adenovirus, Astrovirus, Enterovirus, Parvovirus, Rotavirus, Sapovirus, Influenza, Parainfluenza, RSV, HSV, FSME, Mumps, Measles and Malaria.





Virology

Adenovirus

Product	Description	Matrix	Tests	Art. No.
Real-time RT-PCR				
RIDA®GENE Adenovirus	Multiplex real-time PCR for the direct qualitative detection of Adenovirus in human throat washes, sputum, BAL and stool samples	Throat washes/ sputum/ BAL/stool	100	PG1005
RIDA®GENE Viral Stool Panel I	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus, Adenovirus 40/41 and Astrovirus in human stool samples	Stool	100	PG1315
RIDA®GENE Viral Stool Panel II	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Rotavirus, Adenovirus 40/41 and Astrovirus in human stool samples	Stool	100	PG1325
RIDA®GENE Viral Stool Panel III	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus and Adenovirus 40/41 in human stool samples	Stool	100	PG1335
Enzyme immunoassay				
RIDASCREEN® Adenovirus	Enzyme immunoassay for the detection of Adenoviruses in human stool samples	Stool	96	C1001
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Adenovirus Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP1004
Rapid tests				
RIDA®QUICK Rotavirus/Adenovirus Combi	Immunochromatographic rapid assay for the detection of Rotaviruses and/or Adenoviruses in human stool samples Box with strips	Stool	25	N1002
RIDA®QUICK Rotavirus/Adenovirus Combi	Immunochromatographic rapid assay for the detection of Rotaviruses and/or Adenoviruses in human stool samples Single pouched cassettes	Stool	20	N1003
RIDA®QUICK Rotavirus/Adenovirus/Norovirus Combi	Immunochromatographic rapid assay for the detection of Rotaviruses and/or Adenoviruses and/or Noroviruses genogroup I and II in human stool samples Single pouched cassettes	Stool	20	N1903
Controls for RIDA®QUICK				
RIDA®QUICK Rotavirus/Adenovirus Combi Control	Positive control	–	1.8 ml	NP1904
Sample diluent for RIDA®QUICK				
Rotavirus/Adenovirus Sample diluent	Tubes with 1.5 ml sample diluent	Stool	25	ZN1004





Virology

Astrovirus

Product	Description	Matrix	Tests	Art. No.
Real-time RT-PCR				
RIDA®GENE Viral Stool Panel I	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus, Adenovirus 40/41 and Astrovirus in human stool samples	Stool	100	PG1315
RIDA®GENE Viral Stool Panel II	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Rotavirus, Adenovirus and Astrovirus 40/41 in human stool samples	Stool	100	PG1325
Enzyme immunoassay				
RIDASCREEN® Astrovirus	Enzyme immunoassay for the detection of Astroviruses in human stool samples	Stool	96	C1301
Reference control for RIDASCREEN® ELISA				
RIDASCREEN® Astrovirus Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP1304



Cytomegalovirus

Real-time RT-PCR				
RIDA®GENE CMV	Multiplex real-time PCR for the direct qualitative and quantitative detection of CMV in human plasma (EDTA) and urine samples	Plasma (EDTA)/ Urine	100	PG9005



Tick-borne Encephalitis

Enzyme immunoassays				
RIDASCREEN® FSME/TBE IgG	Specific detection of IgG or IgM antibodies against Tick-borne Encephalitis (TBE) virus	Serum	96	K3421





Virology

Enterovirus

Product	Description	Matrix	Tests	Art. No.
Enterovirus	Real-time RT-PCR			
RIDA®GENE Enterovirus	Multiplex real-time RT-PCR for the direct qualitative detection of Enterovirus (Poliovirus, Echovirus, Coxsackievirus, human Enterovirus 70/71) in human stool samples and CSF	Stool/CSF	100	PG4705



Epstein-Barr-Virus

Enzyme immunoassays				
SeraSpot® Anti-EBV-4 IgG	Specific detection of IgG antibodies against Epstein-Barr-Virus	Serum/ plasma	96	SP-013-4 G-S12
SeraSpot® Anti-EBV-3 IgG	Specific detection of IgM antibodies against Epstein-Barr-Virus	Serum/ plasma	96	SP-013-3 M-S12



Influenza

Real-time RT-PCR				
RIDA®GENE Flu	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Influenza A, Influenza B and H1N1v in human nasal swabs and throat swabs	Nasal swab/ throat swab	100	PG0505
RIDA®GENE Flu & RSV	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Influenza A, Influenza B and RSV in human nasal and throat swabs and BAL	Nasal swab/ throat swab/BAL	100	PG0545





Virology

Hantavirus

Product	Description	Matrix	Tests	Art. No.
Enzyme immunoassays				
RIDASCREEN® Hantavirus Dobrava/ Hantaan IgG	Specific detection of IgG or IgM antibodies against the Dobrava and Hantaan serotype of Hantavirus	96	Serum	K9121
Hantavirus Dobrava/ Hantaan IgM		96	Serum	K9131
RIDASCREEN® Hantavirus Puumala IgG	Specific detection of IgG or IgM antibodies against the Puumala serotype of Hantavirus	96	Serum	K9221
Hantavirus Puumala IgM		96	Serum	K9231



Measles

Masern	Enzyme immunoassays			
RIDASCREEN® Masern/Measles Virus IgG	Specific detection of IgG or IgM antibodies against Measles virus. IgG-analysis in international units (mIU/ml)	Serum	96	K5421
Masern/Measles Virus IgM		Serum	96	K5431



Mumps

Mumps	Enzyme immunoassays			
RIDASCREEN® Mumps Virus IgG	Specific detection of IgG or IgM antibodies against Mumps virus	Serum	96	K5521
Mumps Virus IgM		Serum	96	K5531





Virology

Norovirus

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Hospital Stool Panel	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus (genogroup I and II), Rotavirus and Clostridium difficile toxin genes A (tcdA) and B (tcdB) in human stool samples	Stool	100	PG0705
RIDA®GENE Norovirus	Multiplex real-time RT-PCR for the direct qualitative detection of Norovirus (genogroup I and II) in human stool samples	Stool	100	PG1405
RIDA®GENE Norovirus I & II	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus genogroup I and genogroup II in human stool samples	Stool	100	PG1415
RIDA®GENE Norovirus GI/GII	Multiplex real-time RT-PCT for the simultaneous qualitative detection and differentiation of norovirus genogroup I (GI) and II (GII) nucleic acid	Stool	100	PG1445*
RIDA®GENE Viral Stool Panel I	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus, Adenovirus 40/41 and Astrovirus in human stool samples	Stool	100	PG1315
RIDA®GENE Viral Stool Panel III	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus and Adenovirus 40/41 in human stool samples	Stool	100	PG1335
Enzyme immunoassays				
RIDASCREEN® Norovirus	Enzyme immunoassay for the detection of Noroviruses genogroup I and II in human stool samples	Stool	96	C1401
RIDASCREEN® Norovirus	Enzyme immunoassay for the detection of Noroviruses genogroup I and II in human stool samples	Stool	96	C1401US*
Reference controls for RIDASCREEN® ELISA				
RIDASCREEN® Norovirus Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP1404
Rapid test				
RIDA®QUICK Norovirus	Immunochromatographic Lateral flow rapid assay for the detection of Noroviruses genogroup I and II in human stool sample Single pouched cassettes	Stool	25	N1402
RIDA®QUICK Rotavirus/Adenovirus/Norovirus Combi	Immunochromatographic rapid assay for the detection of Rotaviruses and/or Adenoviruses and/or Noroviruses genogroup I and II in human stool sample Single pouched cassettes	Stool	20	N1903
Controls for RIDA®QUICK				
RIDA®QUICK Norovirus Control	Positive control	–	1.8 ml	NP1404



* Only for sale in the US.



Virology


Parainfluenza

Product	Description	Matrix	Tests	Art. No.
Parainfluenza				
Real-time RT-PCR				
RIDA®GENE Parainfluenza	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of human Parainfluenza 1, 3 and 2/4 in human swabs (nose, throat, nasopharyngeal)	Nasal swab/ throat swab/naso- pharyngeal swab	100	PG5805



Parvovirus

Enzyme immunoassays				
RIDASCREEN® Parvovirus B19 IgG Parvovirus B19 IgM	Specific detection of IgG or IgM antibodies against Parvovirus B19. Detection of antibodies against recombinant VP1 and VP2. Differentiation between acute and past infection with Parvovirus B19 IgG-analysis in international units (IU/ml)	Serum Serum	96 96	K6021 K6031
Microspot-Arrays				
SeraSpot® Anti-Parvovirus-6 IgG	Specific detection of IgG antibodies against Parvovirus	Serum/ plasma	48	SP-012-6 G-S6
SeraSpot® Anti-Parvovirus-5 IgM	Specific detection of IgM antibodies against Parvovirus	Serum/ plasma	48	SP-012-5 M-S6
Line blots				
RIDA® LINE Parvovirus B19 IgG Parvovirus B19 IgM	Line blots for specific detection of IgG or IgM antibodies against Parvovirus B19 with recombinant antigens. Line blots allow differentiation between acute and past infection with Parvovirus B19. Indicative for a probably persistent Parvovirus B19 infection	Serum Serum	20 20	LB6023 LB6033





Virology

Rotavirus

Product	Description	Matrix	Tests	Art. No.
Real-time PCR				
RIDA®GENE Hospital Stool Panel	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus (genogroup I and II), Rotavirus and Clostridium difficile toxin genes A (tcdA) and B (tcdB) in human stool samples	Stool	100	PG0705
RIDA®GENE Viral Stool Panel I	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus, Adenovirus 40/41 and Astrovirus in human stool samples	Stool	100	PG1315
RIDA®GENE Viral Stool Panel II	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Rotavirus, Adenovirus 40/41 and Astrovirus in human stool samples	Stool	100	PG1325
RIDA®GENE Viral Stool Panel III	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Norovirus, Rotavirus and Adenovirus 40/41 in human stool samples	Stool	100	PG1335
Enzyme immunoassay				
RIDASCREEN® Rotavirus	Enzyme immunoassay for the detection of Rotaviruses in human stool samples	Stool	96	C0901
Reference control for RIDASCREEN® ELISA				
RIDASCREEN® Rotavirus Reference Controls	Reference controls A and B	–	2.0 ml (A) 2.0 ml (B)	CRP0904
Rapid tests				
RIDA®QUICK Rotavirus	Immunochromatographic rapid assay for the detection of Rotaviruses in human stool samples Single pouched cassettes	Stool	20	N0903
RIDA®QUICK Rotavirus/Adenovirus Combi	Immunochromatographic rapid assay for the detection of Rotaviruses and/or Adenoviruses in human stool samples Single pouched cassettes	Stool	20	N1003
RIDA®QUICK Rotavirus/Adenovirus/Norovirus Combi	Immunochromatographic rapid assay for the detection of Rotaviruses and/or Adenoviruses and/or Noroviruses genogroup I and II in human stool samples Single pouched cassettes	Stool	20	N1903
Controls for RIDA®QUICK				
RIDA®QUICK Rotavirus/Adenovirus Combi Control	Positive control	–	1.8 ml	NP1904
Sample diluent for RIDA®QUICK				
Rotavirus/Adenovirus Sample diluent	Tubes with 1.5 ml sample diluent	Stool	25	ZN1004





Virology

Respiratory Syncytial Virus & Human Metapneumovirus

Product	Description	Matrix	Tests	Art. No.
RSV & hMPV				
Real-time RT-PCR				
RIDA®GENE RSV & hMPV	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of RSV and hMPV from human swabs (nose, throat, nasopharyngeal), throat washes and BAL	Nasal swab/ throat swab/naso- pharyngeal swab/throat washes/BAL	100	PG5905
RIDA®GENE Flu & RSV	Multiplex real-time RT-PCR for the direct qualitative detection and differentiation of Influenza A, Influenza B and RSV from human swabs (nose, throat) and BAL	Nasal swab/ throat swab/BAL	100	PG0545



Sapovirus

Sapovirus				
Real-time RT-PCR				
RIDA®GENE Sapovirus	Multiplex real-time RT-PCR for the direct qualitative detection of Sapovirus in human stool samples	Stool	100	PG1605





Virology

Accessories

Product	Description	Matrix	Tests	Art. No.
Accessories				
Color compensation				
RIDA®GENE Color Compensation Kit I	To generate a Color Compensation File for 3- and 4-plex RIDA®GENE real-time PCR experiments on the LightCycler® 480II*	–	3	PG0001
RIDA®GENE Color Compensation Kit IV	To generate a Color Compensation File for RIDA®GENE real-time PCR experiments on the LightCycler® 480II**	–	3	PG0004
Accessory				
DNA/RNA extraction				
RIDA® Xtract	Spin-filter based extraction kit for the simultaneous isolation and purification of DNA and RNA in various matrices (serum/ plasma/ cerebral fluid/ cell culture supernatant/ other cell free body fluids (e.g. urine)/ swabs/tissue biopsies/stool)	see description	250 preparations	PGZ001
Accessory for RIDASCREEN® antibody detection tests				
RIDA® RF-Absorbens	Anti-human IgG for absorption of rheumatoid factors (RF) and IgG antibodies in human serum or plasma	Serum/ plasma	100	Z0202



* For RIDAGENE products of the generation 1.0.

** For RIDAGENE products of the generation 2.0.



Systems

R-Biopharm offers a wide and flexible range of automation and software solutions for individual laboratory needs.

Due to time and cost reasons, automation plays an increasingly important role in clinical laboratories. Each diagnostic has specific needs and demands that must be adapted to the laboratory's requirements. This is where R-Biopharm comes in with its solutions for automation. In cooperation with renowned partners, we offer equipment and software solutions from small to high sample throughput for the different laboratory requirements.

Systems & software

R-Biopharm offers different platforms for ELISA, PCR and rapid tests.

The lateral flow reader RIDA®QUICK SCAN II offers additional security for the analysis and documentation of your rapid tests.

For molecular diagnostics R-Biopharm offers the automated interpretation software RIDA®SEEK for RIDA®GENE real-time PCR kits. RIDA®SEEK enables qualitative and quantitative interpretation of results from PCR cycler raw data.

All R-Biopharm ELISA tests are verified on various automation solutions. Further we provide convenient software solutions for measurement, evaluation and documentation of RIDASCREEN® ELISA tests and RIDA qLine®.

Services

Our application specialists continuously improve, update and validate our systems and devices. Moreover, our goals are to accompany you as a reliable partner during the process of planning, installation and also later in your daily routine.

Systems

Molecular diagnostics

Product	Description	Units		Art. No.
RIDA®CYCLER	qPCR thermocycler 4 channels, incl. 1 box with reaction tubes,	1	–	ZRCYCLER
RIDA®SEEK	Software for evaluation and documentation of RIDA®GENE real-time PCR kits	1	–	ZRIDASEEK

Immunoassay systems and evaluation software

ELISA-systems				
Dynex DS2®	Fully automated 2-microtiter plate analyzer with 2 incubators	1	–	Z62000
Dynex DSX®	Fully automated 4-microtiter plate analyzer with 2/4 incubators	1	–	Z65200 Z65400
Dynex Agility®	Fully automated 12-microtiter plate analyzer with 12 incubators	1	–	ZAGILITY
ELISA washer, reader and evaluation software				
RIDA®ABSORBANCE 96	Microtiterplate Reader	1	–	ZRA96
BioTek® 50™ TS 8V	Microtiterplate Washer	1	–	Z50TS8V
BioTek® 800™ TS	Microtiterplate Reader	1	–	Z800TS
RIDASOFT® Win.NET	Software for measurement, evaluation and documentation of RIDASCREEN® ELISA tests	1	–	Z9996
RIDASOFT® A.M.Sys	Software for the input, measurement, evaluation and documentation of the RIDASCREEN® Allergy ELISA Tests	1	–	Z9997

Rapid tests

RIDA®QUICK SCAN II - IVD SET	Lateral flow reader (CE-IVD) and 2D barcode scanner	1	–	ZRQS2-KD-SET
RIDA®QUICK SCAN II	Lateral flow reader (CE-IVD)	1	–	ZRQS2-KD



Systems


Blot systems and evaluation software

Product	Description	Units		Art. No.
RIDA qLine® autoBlot	Fully automated analyzer for 36 RIDA qLine® Allergy test strips	1	–	ZG3101
RIDA qLine® Orbital Shaker	Orbital shaker (100 - 240V)	1	–	ZG2601
RIDA qLine® Scan	Reader for RIDA qLine® Allergy (CE-IVD)	1	–	ZG1109
RIDA qLine® QC-Kit	10 test strips for function control of the evaluation unit	1	–	ZG1108
RIDA qLine® SOFT	Software for measurement, evaluation and documentation of RIDA qLine® test strips	1	–	Z9995

Microspot array diagnostics

<i>SpotSight</i> ® strip	Scanner for image acquisition and interpretation (strip)	1	–	Z-SP-STRIP-B
<i>SpotSight</i> ® plate mono	Scanner for image acquisition and interpretation (plate)	1	–	Z-SP-PLATE-C

The R-Biopharm Group – contact us

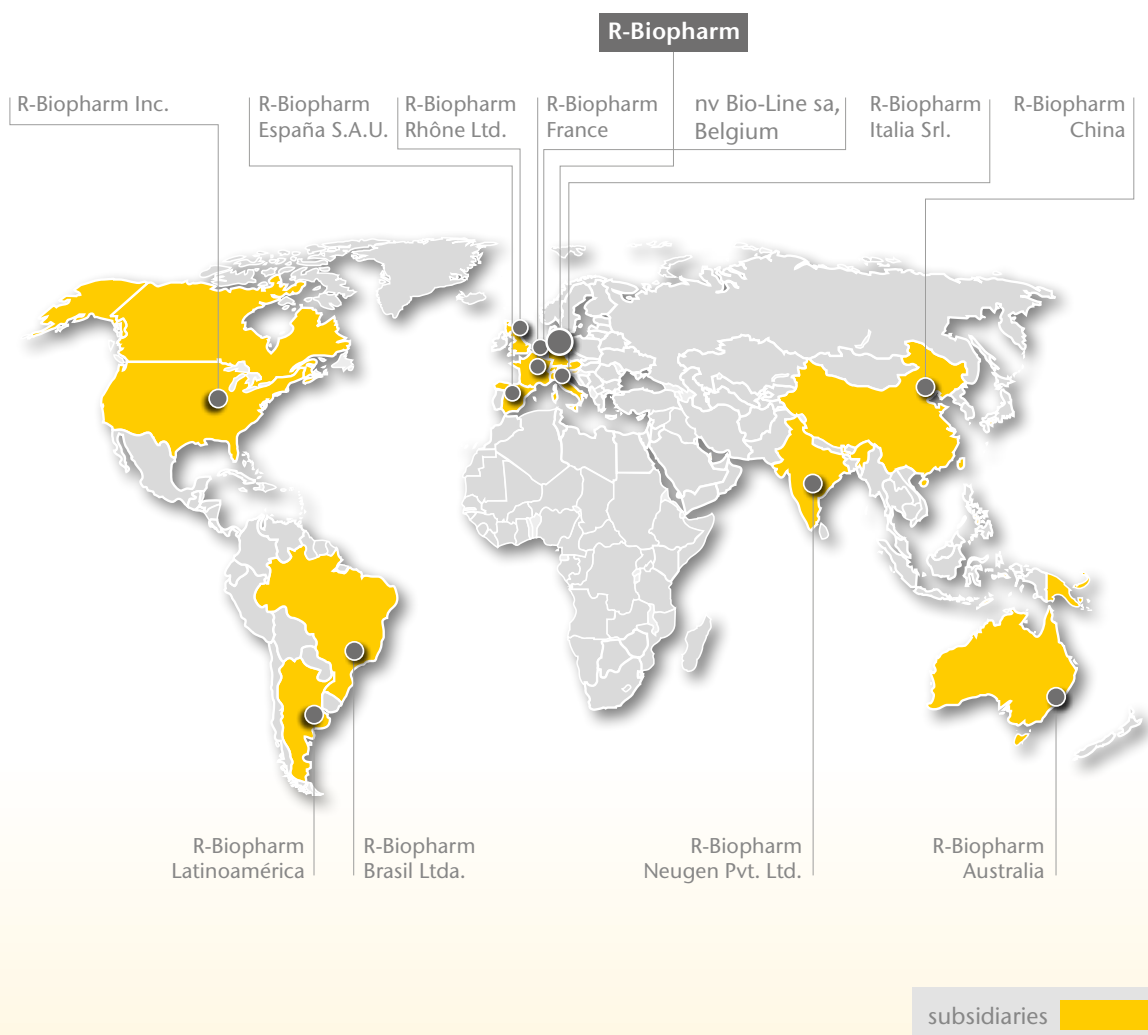

R-Biopharm

An der neuen Bergstraße 17
64297 Darmstadt, Germany
Phone: +49 (0) 61 51 - 81 02-0
Fax: +49 (0) 61 51 - 81 02-40
E-mail: info@r-biopharm.de,
csi@r-biopharm.de

www.r-biopharm.com

General terms & conditions of R-Biopharm AG

(Date of Issue: October 2010)

I. General Provisions

These General Terms & Conditions only are valid for entrepreneurs, legal entities under public law or public-law special assets (legal entities according to § 310 I German Civil Code ("Bürgerliches Gesetzbuch" - "BGB"). We deliver according to these General Terms & Conditions exclusively. They are deemed to have been acknowledged with the placing of an order or the receipt of the goods and shall also apply to all future business relationships, even if they are not explicitly agreed upon again. Deviating Terms and Conditions are not binding for us, even if we do not object to them explicitly.

II. Orders and Offer Documents

Our offers are subject to alteration. Decisive for the scope of our delivery obligation are our offer in writing respectively our written order confirmation. Deliverable are only the products which are contained in our current applicable price lists.

III. Prices and Conditions of Payment/Withdrawal in case of default

1. Purchase price is the price stated by us or - if no price has been stated - the price which is contained in our price list, which is in effect on the day of the order. The prices stated by us - unless otherwise stipulated in writing - are including packing and shipping costs, excluding VAT. The deduction of cash discounts shall not be granted. A small-quantity surcharge in the amount of 10 Euros can be charged for deliveries with a product value of up to 300 Euros (small quantity).
2. Payment obligations resulting from the delivery of goods are to be fulfilled within thirty (30) days of the invoice date by bank transfer exclusively and shall be deemed to have been effected only to the extent, to which we can dispose of them freely at a bank. For checks and bills of exchange, a processing fee of 30 Euros shall be charged; discounting and expenses shall be for the account of the Buyer.
3. The Buyer shall only be entitled to set-off with a counter-claim which is undisputed or has been determined by a final verdict. A right of retention the Buyer does only have as far as it is resulting from the same contractual relationship.
4. Should the Buyer be in default with due payments entirely or partly, the regulations of the statutory law are applicable. Interest in the amount of 8% above the basic interest rate (as it is published by the German Federal Bank) shall be due. We are reserving the right to claim any exceeding damage for delay.
5. In case of withdrawal, we are entitled - at the expense of the Buyer - to let the goods, which have been delivered by us, mark, store separately and collect. The Buyer - already yet - is declaring his consent that the persons who are commissioned with the collection are entitled to access the premises, on which the goods are, and enter them by car for this purpose.
6. In case of our withdrawal, we are not obliged to further deliveries any more, also regarding further future deliveries.

IV. Retention of Title

1. We shall retain title to the goods delivered by us, until all the claims, to which we are entitled on whatever legal grounds arising from our business relationship with the Buyer, have been fully satisfied. Upon the Buyer's request, we shall be obligated to release the securities in so far as their realizable value exceeds our claims by more than 10%. We reserve the right to select the items of collateral to be released.
2. The Buyer undertakes to only sell the goods, which are subject to retention, in his ordinary course of business, according to his usual terms and conditions of business and only as long as he is not in default with his payments. He is entitled to resell the goods, which are subject to retention, only on the condition that a transfer of the receivables, resulting from such a resale, to us takes place. He is not be entitled to dispose of the goods, which are subject to retention, in any other way (such as e. g. collateral assignment, pledging, leasing, lending, etc.). The Buyer is obligated to immediately notify us of any seizure or other interference by a third party, together with handing over of the documents which are necessary for an intervention.

V. Delivery

1. Our delivery times are generally only approximate and not binding.
2. Uncontrollable incidents, for which we are not responsible, e. g. natural phenomena, war, orders of the authorities, embargo, unexpected delays in the delivery of essential components and other materials ("Force Majeure"), shall prolong the delivery time reasonably. This also applies, if these incidents occur during a delay in delivery or at a sub-supplier. However, the delivery time shall be prolonged by a maximum period of two (2) months. Should we also not be able to deliver after this time, then the Buyer as well as we ourselves are entitled to withdraw from the contract. Any claims of damages of the Buyer for this reason are excluded. Should we withdraw from the contract, we shall immediately refund the Buyer any and all payments possibly rendered for not yet delivered goods.
3. Should the Buyer - despite reminder - not fulfill his payment obligations resulting from existing contracts, we shall only supply on advance payment from then on.
4. We are entitled to partial deliveries to a reasonable extent; here each partial delivery can be invoiced separately. In case of order on call, the call-off has to take place at least two (2) calendar weeks prior to the desired delivery date.

VI. Shipment and Passing of Risk

1. Dispatch ex works or distribution warehouse shall be carried out at the expense of the Buyer. Shipping route and mode of dispatch shall be determined by us. We shall only be obligated to obtain a transport insurance, if explicitly instructed to do so by the Buyer in writing; the Buyer shall bear the costs for this insurance.

2. The passing of risk to the Buyer takes place as soon as the goods have been handed over to the haulage contractor respectively leave our factory or distribution warehouse for the purpose of dispatch; this also is valid, if we - by way of exception - organize additional services, e. g. carriage prepaid shipping, delivery to the premises of the Buyer, or similar. In particular we are not liable for alteration or deterioration of the goods during transport or resulting from improper storage. Should we have notified the Buyer that the goods are ready for dispatch or collection, the risk passes on to the Buyer, if he does not have the goods delivered or collect them, despite of us having set him a reasonable period of time for doing so; regarding that, the passing of risk takes place at the beginning of the day which follows the day, on which the deadline has expired.

VII. Warranty/Liability

1. It is precondition for the execution of claims based on a defect, that the Buyer has performed his responsibilities to examine and complain according to § 377 of the German Commercial Code ("Handelsgesetzbuch" - "HGB") correctly and completely.
2. We are liable for faultlessness of the goods corresponding to the state of the art. Features of samples and specimens as well as any statements regarding the condition of the goods, shall only be considered as an agreement on quality, if they explicitly have been agreed upon as determining the condition of the goods. Otherwise they are non-binding and do not free the Buyer from an own inspection of the goods concerning their suitability for his purposes. We neither grant guarantees with the content of a liability without fault nor any other kind of guarantees for quality and durability in the legal sense.
3. We are not liable for damages as far as they have been caused by improper storage of our products and/or their application contrary to the prescriptions - e. g. application after expiry of their shelf life or contrary to the direction for use - or as far as they have been caused by the Buyer in any other way.
4. The exceeding of use-by dates after the delivery does not entitle the Buyer to claims of any kind, but is deemed to be the usual condition. This is not the case, if the period between the date of delivery and the use-by date is less than four (4) calendar weeks.
5. We shall only be liable for damages, as far as we attributable have caused them by intent or gross negligence (disregard for the due care and attention to a very coarse extent); except in case of violation of essential contractual obligations (obligations, whose fulfillment enables the proper execution of the contract at all and on whose observance the contractual partner may rely regularly). In this last-mentioned case we are liable for each negligence with the restriction that - in case of violation of essential contractual duties by slight negligence - our liability is limited to the damage which typically is predictable.
6. Should we not have violated any essential contractual obligations in the sense mentioned before, we are not liable in cases of slight negligence. Unaffected by any limitation of liability contained in these General Terms & Conditions stay: Liability for intent, malice, initial inability, gross negligence, liability resulting from a guarantee (which, however, we generally not grant), bodily harms and other cases of legally compelling liability - in these cases the statutory law is valid (under exclusion of the Terms and Conditions of our contractual partner).
7. The regulations of this clause Warranty/Liability are valid for our contractual liability as well as liability resulting from tort (unaffected thereby stays the action for possession in case of tort, after statutory limitation has taken place, § 852 German Civil Code ("Bürgerliches Gesetzbuch" - "BGB")).
8. As far as our liability is excluded or limited, this shall also apply to the personal liability of our representatives, employees and vicarious agents and our liability for them.
9. As far as there is a defect of the goods, for which we are liable, the Buyer has to grant us the opportunity to execute subsequent performance within a term of generally two (2) calendar weeks, before the assertion of his further rights. In case that subsequent performance fails twice, in case of our refusal, or if subsequent performance is impossible, is delayed unreasonably or unreasonable for the Buyer due to other reasons, the Buyer may - according to his choice - execute his further legal rights, namely rescission or reduction of the purchase price and (regarding defects for which we are liable) claim of possibly occurred damages or compensation for possible futile expenditure, by which our liability is limited according to the preceding regulations.

VIII. Burden of Proof/Export/Effectiveness

1. With none of the stipulations of these General Terms & Conditions an alteration of the burden of proof is intended.
2. We are not liable for the correctness of information regarding foreign-trade which we provide to our best conscience; it is the Buyer's responsibility to assess the compliance with foreign-trade regulations with regard to our products himself.
3. Should any of the regulations of our General Terms & Conditions be ineffective and/or incomplete, the validity of the other regulations shall remain unaffected thereby.

IX. Applicable Law and Place of Jurisdiction

1. The contractual relationship shall be governed by the laws of the Federal Republic of Germany, which shall be applicable supplementary. The UN-convention on contracts regarding the International Sale of Goods (CISG) shall not apply.
2. Exclusive Place of Jurisdiction is Darmstadt (Germany). However, we are entitled to file a lawsuit against the Buyer also at any other court, which does have jurisdiction regarding him according to the general regulations.



R-Biopharm

An der neuen Bergstraße 17
64297 Darmstadt, Germany
Phone: +49 61 51 - 81 02-0
Fax: +49 61 51 - 81 02-40
E-mail: info@r-biopharm.de
www.r-biopharm.com