





Kit components:

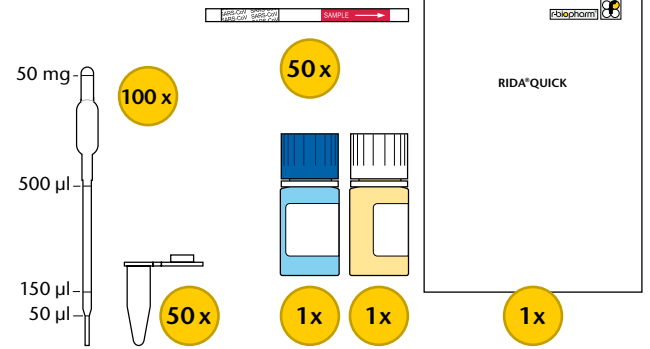

RIDA® QUICK Procedure Card SARS-CoV-2 Antigen

1


Test and sample preparation



Collect sample (swab in transport medium)
Bring the kit to 20 - 25 °C


2

Sample preparation




50 µl Reagent A

3



50 µl Reagent B

4




50 µl sample in transport medium with pipet

5


Mixing & incubation

Mix




6

10 min




7

Sample testing




8

10 min



9

Test interpretation

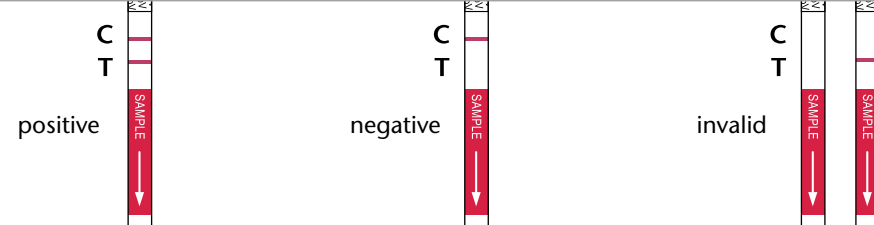

positive negative invalid

Please consult the instructions for use for complete instructions!